




Atrium Oasis Dry Suction Water Seal Chest Drain

GETINGE

Set-up

Set-up

Open floor stand for set-up. Move the patient tube clamp next to the in-line connector for set-up convenience and patient safety. Follow steps 1-4 and refer to additional details concerning system set-up and operation.

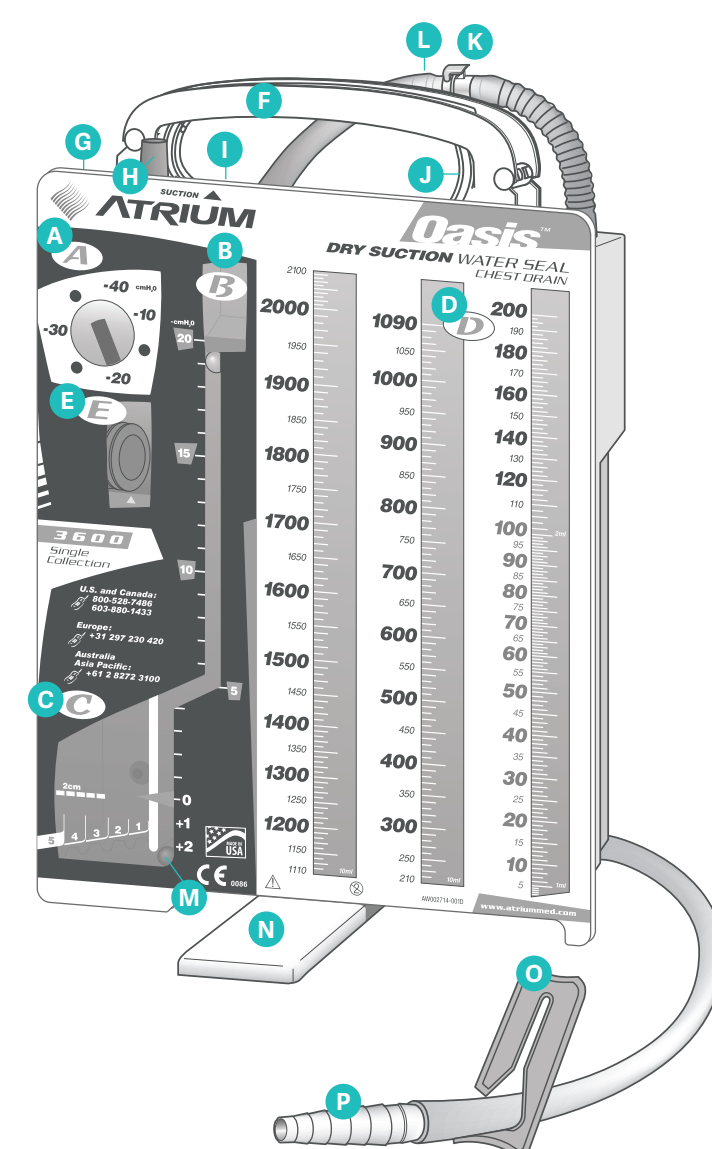


- A** Dry Suction Regulator
- B** Water Seal Chamber
- C** Air Leak Monitor
- D** Collection Chamber
- E** Suction Monitor Bellows
- F** Easy-to-Grip Handle
- G** Positive Pressure Release Valve
- H** Suction Port
- I** Manual High Negativity Vent
- J** Multi-position Hangers
- K** In-line Connector
- L** Needleless Access Port
- M** Patient Pressure Float Ball
- N** Swing Out Floor Stand
- O** Patient Tube Clamp
- P** Patient Connector


Step 1

Fill water seal **B** to 2 cm line

Add 45 ml of sterile water or sterile saline via the blue suction port located on top of the drain. For models available with sterile fluid, twist top off bottle and insert tip into suction port. Squeeze contents into water seal until fluid reaches 2 cm fill line.

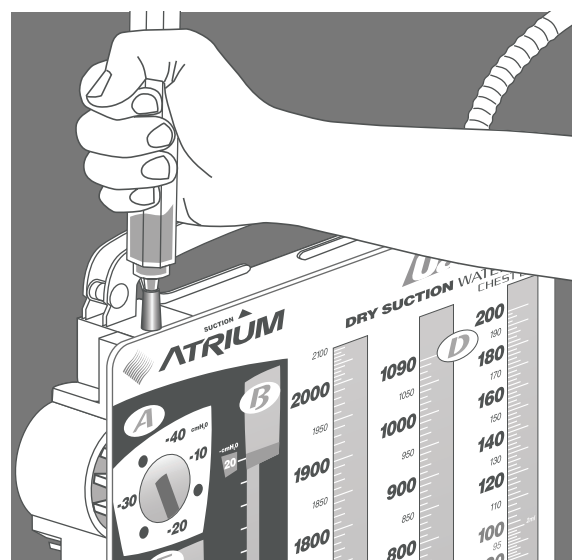


Once filled, water becomes tinted blue for visibility of air leaks and convenient monitoring of patient pressures.

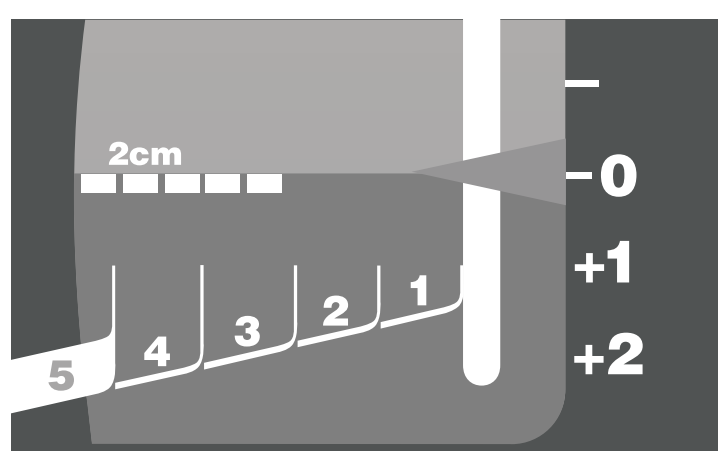

Step 2

Connect chest drain to patient

Connect chest drain to patient prior to initiating suction.

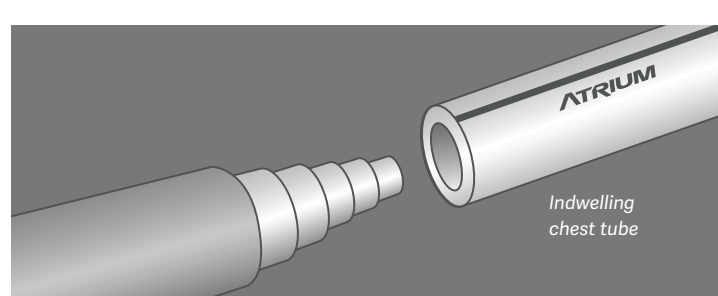

Step 3

Connect suction to chest drain

Attach suction line to the blue suction port on top of chest drain.


Suction source

The suction source should provide a *minimum vacuum pressure of -80 mmHg* at 20 liters of air flow per minute for chest drain operating efficiency at a suction control setting of -20 cmH₂O. The suction source vacuum should be greater than -80 mmHg when multiple chest drains are connected to a single suction source.

Step 4


Turn suction source on

Increase suction source vacuum to -80 mmHg or higher. Suction regulator is preset to -20 cmH₂O. Adjust as required.

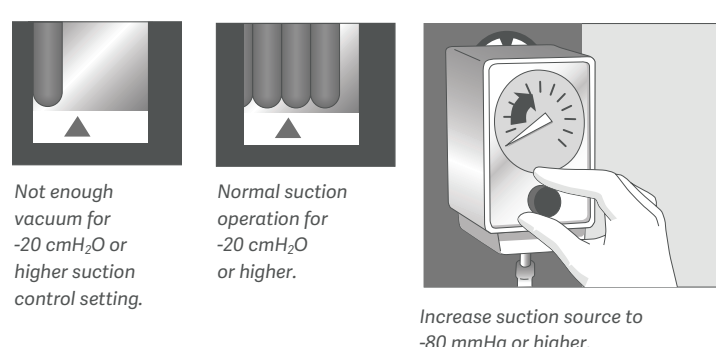


Suction monitor bellows

When the suction control regulator is set at -20 cmH₂O or higher, the bellows must be expanded to the **▲** mark or beyond when suction is operating. If the bellows is observed to be expanded, but less than the **▲** mark, the suction source vacuum pressure must be increased to -80 mmHg or higher. For a regulator setting less than -20 cmH₂O suction (-10 cmH₂O), any observed bellows expansion across the monitor window will confirm suction operation. The bellows need not be expanded to the **▲** mark for pressures less than -20 cmH₂O, just visibly expanded to confirm suction operation.

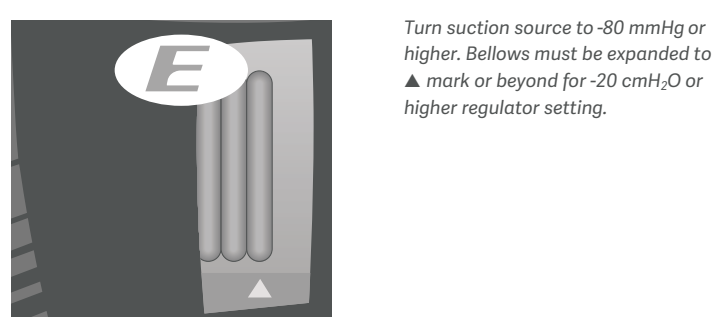

Continually adjustable dry suction control

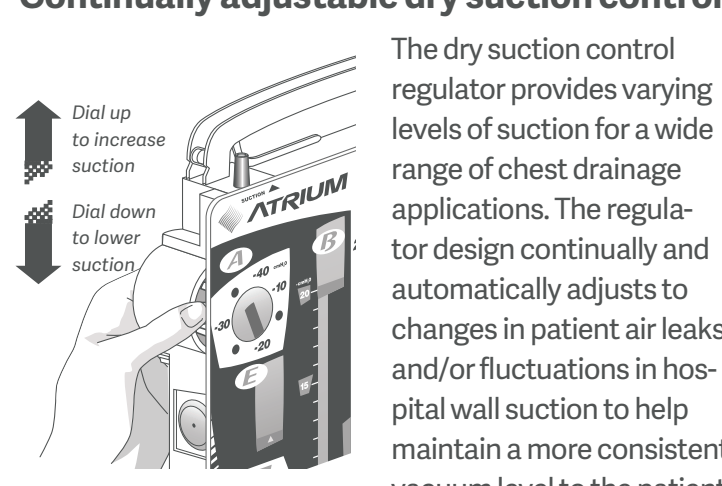


The dry suction control regulator provides varying levels of suction for a wide range of chest drainage applications. The regulator design continually and automatically adjusts to changes in patient air leaks and/or fluctuations in hospital wall suction to help maintain a more consistent vacuum level to the patient.

Suction pressure can be set to any desired pressure level between -10 cmH₂O and up to a maximum of -40 cmH₂O. Changing the suction pressure is accomplished by adjusting the rotary dry suction control dial located on the side of the drain. Dial down to lower the suction setting and dial up to increase the suction pressure setting.

In-line patient tube connector


The locking in-line patient tube connector provides system replacement, simple disconnection after use, and rapid in-line ATS blood bag attachment when required. The in-line connector must remain **securely connected at all times** during operation and patient connection. **Tube clamp must be closed prior to in-line connector separation.**

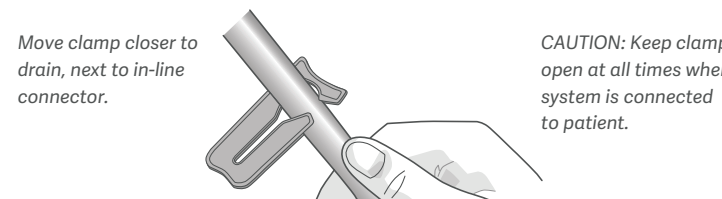

What to check during system operation

Verifying suction operation via the suction monitor bellows

The bellows located in the suction monitor window will expand only when suction is operating. The bellows will not expand when suction is not operating or is disconnected. The **▲** mark allows quick and easy confirmation of vacuum operation over a wide range of continuously adjustable suction control settings.

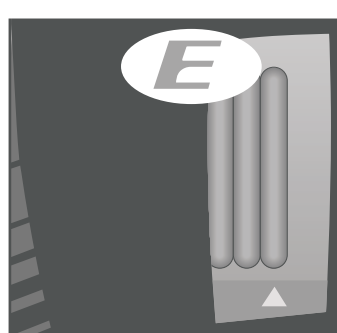


Bellows must be expanded to **▲** mark or beyond for a -20 cmH₂O or higher regulator setting.

Increase vacuum source when bellows is not expanded to **▲** mark

If the bellows is observed to be expanded, but less than the **▲** mark, the vacuum source pressure must be increased to -80 mmHg or higher.

Changing suction pressures

Changing suction pressure is accomplished by adjusting the rotary dry suction control dial located on the side of the drain. Dial **down** to lower the suction pressure and dial **up** to increase the suction pressure.

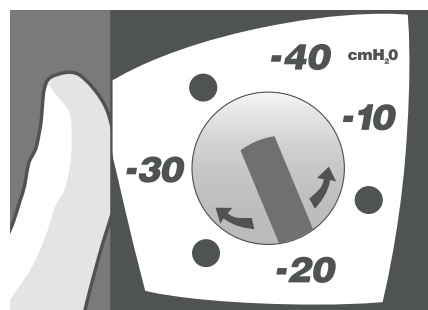

NOTE: When changing suction pressure from a higher to lower level, use of the manual high negativity vent after regulator adjustment will reduce excess vacuum pressure down to the lower prescribed level.

Verifying water seal operation

The water seal must be filled and maintained at the 2 cm level to ensure proper operation and should be checked regularly when used for extended periods. As required, additional water may be added by a 20 gauge or smaller needle and syringe via the grommet located on the back. Fill to the 2 cm line.

Placement of unit

Always place chest drain below the patient's chest in an upright position. To avoid accidental knock-over, open the floor stand for secure placement on floor or hang the system bedside with the hangers provided.

Recording drainage volume

The collection chamber incorporates a writing surface with easy-to-read fluid level graduations. Please refer to individual product inserts for specific model graduations.

Observing water seal for patient air leaks

The chest drain offers air leak detection with rapid air leak assessment and enhanced visibility due to the tinted water. When air bubbles are observed going from **right to left** in the air leak monitor, this will confirm a patient air leak.

Continuous bubbling

in the bottom of the water seal air leak monitor will confirm a persistent air leak.

Intermittent bubbling

in the air leak monitor with float ball oscillation will confirm the presence of an intermittent air leak.

No bubbling

with minimal float ball oscillation at bottom of the water seal will indicate no air leak is present.

Observing graduated water seal column for changes in patient pressure

Patient pressure can be determined by observing the level of the blue water and small float ball in the graduated water seal column. With suction operating, patient pressure will equal the suction control setting plus the graduated water seal column level. For gravity drainage (no suction) patient pressure will equal the graduated water seal column level only.

Graduated air leak monitor


For those models with a graduated air leak monitor, air leak bubbling can range from 1 (low) to 5 (high). Air bubbles create an easy to follow air leak pattern for monitoring patient air leak trends.

High negativity float valve

The high negativity float valve, with its controlled release action, enables the thoracic patient to draw as much intrathoracic pressure as is required during each respiratory cycle. During prolonged episodes of extreme negative pressure, a controlled release system will automatically relieve excess vacuum to the lower, prescribed pressure level.

Manual high negativity vent


To lower the height of the water seal column or to lower patient pressure when connected to suction, **depress** the manual vent located on top of the drain until the float valve releases and the water column returns to the desired level. **Do not use manual vent to lower water seal column when suction is not operating or when the patient is on gravity drainage.**

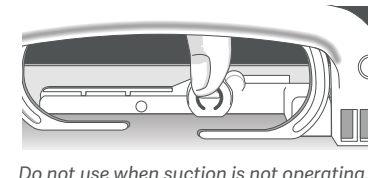

Do not use when suction is not operating.

Positive pressure protection

The positive pressure release valve, located on top of drain, opens to release accumulated positive pressure. **Do not obstruct the positive pressure release valve.**

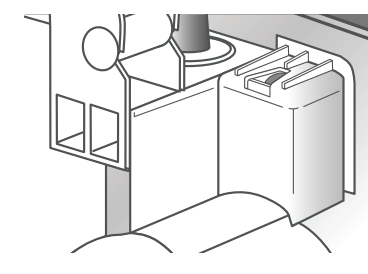

Sampling patient drainage

Sampling of patient drainage must be in accordance with approved hospital infection control standards. Selected models include a needleless Luer port on the patient tube connector for sampling patient drainage. Alcohol swab the Luer port prior to syringe attachment (no needle). Fluid samples can also be taken directly from the patient tube by forming a temporary dependent loop and inserting a 19 gauge needle at an oblique angle. Alcohol swab the patient tube prior to inserting syringe at a shallow angle. **Do not puncture patient tube with an 18 gauge or larger needle.**

System disconnection

For models equipped with an in-line connector, **close the patient tube clamp prior to disconnecting** the chest drain patient tube from patient. Clamp off all indwelling thoracic catheters prior to disconnecting chest drain from patient.


System disposal

Disposal of chest drain and its contents should be in accordance with all applicable regulations.

Problems to check for during CDU use

Potential problems can be avoided by routinely checking the patient, tube connectors, and drainage system at regularly scheduled intervals. Listed below are many of the common problems that can be corrected:

- clot in chest tube inside patient
- clot in the patient tube
- dependent loop in patient tube with fluid
- kink in patient tube from bed rail or patient position
- partial dislodgement of catheter from patient
- partial disconnection of patient tube from chest tube connector
- overfilled water seal (water is above 2 cm line)
- in-line connectors not properly secured
- patient tube clamp may be closed
- floor stand is not fully opened
- chest drain is not upright
- chest drain is not positioned sufficiently below patient's chest
- suction monitor bellows does not fully expand because source suction falls below the minimum operating range or poor connection

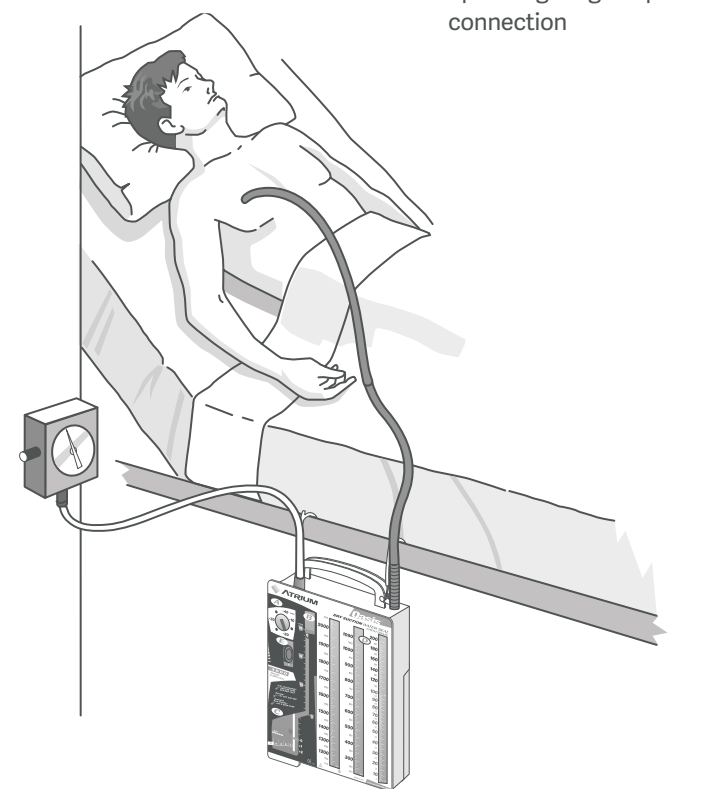


Troubleshooting

How do I determine patient pressure with a dry suction chest drain?

Whether using a traditional wet or dry suction operating system, one cannot overemphasize the importance of the graduated water seal column when it comes to diagnosing the patient's condition or monitoring normal system operation. Patient pressure can be determined by observing the level of the blue water and small float ball in the graduated water seal column. With suction operating and the bellows expanded across the suction monitor window, patient pressure will equal the suction control setting (read directly from the regulator dial) plus the graduated water seal column level. For example, when the suction monitor bellows is expanded to the **▲** mark or beyond to confirm a -20 cmH₂O suction setting, and the graduated water seal column reads -15 cmH₂O, patient pressure is -35 cmH₂O (-20 cmH₂O + -15 cmH₂O = -35 cmH₂O). For gravity drainage (no suction) patient pressure will equal the graduated water seal column only.

What should I do when the suction monitor bellows is not expanded to the **▲** mark when the regulator is set at -20 cmH₂O or higher?

The position of the bellows across the suction monitor window will alert the operator that the suction source has fallen below the minimum operating range for the prescribed suction control setting. Simply increase the vacuum source to -80 mmHg or higher. The suction monitor bellows must expand to the **▲** mark or beyond for -20 cmH₂O or higher suction regulator setting.

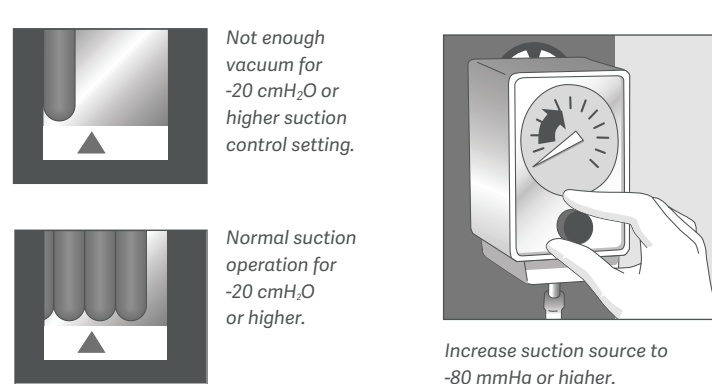

Not enough vacuum for -20 cmH₂O or higher suction control setting.

Normal suction operation for -20 cmH₂O or higher.

Increase suction source to -80 mmHg or higher.

What should I do when the bellows does not fully expand to **▲** the mark after I increase the suction source vacuum?

Dry suction chest drains require higher levels of vacuum pressure and air flow from the suction source to operate properly at each suction control setting as compared to traditional water controlled operating systems. The suction source should provide a minimum vacuum pressure of -80 mmHg at 20 liters of air flow per minute for chest drain operating efficiency at a suction control setting of -20 cmH₂O. The suction source should be greater than -80 mmHg when multiple chest drains are connected to a single suction source. If the bellows does not fully expand to the **▲** mark, it may simply be that the suction source is not functioning to its full potential to provide the minimum vacuum pressure or air flow required to "drive" the suction control regulator. Additionally, conditions may exist that can reduce, or "restrict" air flow from the suction source. A restrictive clamp, connector, or kink in the suction line tubing can potentially "starve" the chest drain of air flow. A leak in a connection or wall canister, along with extensive lengths of suction tubing can also reduce air flow to the unit.

To troubleshoot this situation, first check to be sure that all connections are air-tight. Inspect the suction tubing and connections for possible cracks, leaks, kinks, or occlusion. You may need to simply bypass a "leaky" wall canister. Try connecting the chest drain to a different suction source or wall regulator. When multiple chest drains are "Y" connected to a single suction source, if possible, reconnect the drains to separate suction sources. Finally, replace the chest drain if you suspect the unit is cracked or damaged.

Does the bellows need to expand beyond the **▲** mark for a -10 cmH₂O regulator setting?

No. For a regulator setting less than -20 cmH₂O suction (-10 cmH₂O), any observed bellows expansion across the monitor window will confirm suction operation. The bellows need not be expanded to the **▲** mark for suction pressures less than -20 cmH₂O, just visibly expanded to confirm suction operation.

How do I confirm my patient has an air leak when:

- **There is no bubbling in the water seal?** If there are no air bubbles observed going from right to left in the air leak monitor, there is no patient air leak. In order to confirm that your patient's chest catheter is patent, temporarily turn suction off and check for oscillation of the patient pressure float ball in the water seal column coinciding with patient respiration.
- **Bubbling is present in the water seal?** Whenever **constant or intermittent bubbling** is present in the water seal air leak monitor, this will **confirm an air leak is present**. Oscillation of the patient pressure float ball at the bottom of the water seal **without bubbling will indicate no apparent air leak**. Bubbling from right to left must be present to confirm an air leak. To determine the source of the air leak (patient or catheter connection), **momentarily** clamp the patient tube close to the chest drain and observe the water seal. If bubbling stops, the air leak may be from the catheter connections or the patient's chest. Check the catheter connectors and patient dressing for a partially withdrawn catheter. If bubbling continues after temporarily clamping the patient tube, this will indicate a system air leak requiring system replacement.

What does it mean when the small float ball is located at the bottom of the water seal column?

If the small float ball is located and oscillating at the bottom of the water seal column **with no bubbling**, there is no apparent patient air leak. However, the water seal should be carefully monitored for the presence of an **occasional or intermittent** air leak.

Is it normal for the patient pressure float ball to fluctuate up and down (tidal) near the bottom of the water seal column?

Yes. Once your patient's air leak is resolved, you will generally observe moderate tidaling in the water seal column. Increases in intrathoracic pressure will cause the water level to rise (the ball rises) during patient inspiration and will lower or decrease (the ball drops) during expiration. This diagnostic tool will help to confirm patency of your patient's catheter(s).

Have a question or need help in a hurry? Call Getinge toll free at 1-800-528-7486.

▲ Atrium Oasis, Ocean, and Express are manufactured by Atrium Medical Corporation / 40 Continental Blvd., Merrimack, NH 03054 / Tel. (603) 880-1433. Protected by the following international and U.S. patents: http://patents.maquet.com. © AUCON: Federal (US) law restricts this device to sale by or on the order of a physician. GETINGE and Atrium are trademarks or registered trademarks of Getinge AB, its subsidiaries or affiliates in the United States or other countries. Atrium, Oasis, Ocean and Express are registered with the U.S. Patent and Trademark Office. Copyright 2019 Atrium Medical Corp. All rights not expressly granted are reserved. Refer to Instructions for Use for current indications, warnings, contraindications, and precautions. Printed in U.S.A. -03/19 - PN 010395 REV AB

Sales Office, US - 45 Barbour Pond Drive - Wayne, NJ 07070
Sales Office, Canada 90 Matheson Blvd West, Suite 300 - Mississauga, Ontario L5R 3R3 - Canada

www.getinge.com

MCV00033028 REV B EXP 03/21